

Endothelin-1 ELISA

Enzyme immunoassay for the quantitative determination of endothelin-1 in serum, EDTA plasma, cell culture supernatant and tissue extract

REF

JP27165



12 x 8

For illustrative purposes only.

To perform the assay the instructions for use provided with the kit have to be used.

Distributed by:

Code No. 27165

Endothelin-1 Assay Kit - IBL**INTRODUCTION**

Endothelin-1 (ET-1), a peptide of 21 amino acid residues, is the most potent vasoconstrictor substance known. The discovery by Rubanyi's group in 1985 of a peptide termed endothelium-derived contracting factor (EDCF) and the isolation, sequencing, cloning and naming endothelin by Yanagisawa of the most potent vasoconstrictor has led to more understanding of many physiological effects. ET-1 is known to be one of a family of three mammalian vasoactive peptides including endothelin-2 (ET-2) and endothelin-3 (ET-3). These related peptides differ from ET-1 at the two and six amino acid residue positions, respectively. Those genes make three pre-propeptides that are cleaved into three big endothelin molecules, each 39 amino acid long. A number of reviews of function, molecular biology of the endothelin family of peptides and propeptides are available. ET-1 has been shown to have potent effects on smooth muscle cells, fibroblasts and to be involved in many disease processes, particularly cardiovascular diseases. It has been shown to be important in congestive heart failure, renal failure and pulmonary hypertension. Human ET-1 has identical amino acid sequence to bovine, canine, murine, porcine, rabbit and rat ET-1.

PRINCIPLE

This kit is a solid phase sandwich ELISA using 2 kinds of high specific antibodies. Tetra Methyl Benzidine (TMB) is used as coloring agent (Chromogen). The strength of coloring is in proportion to the quantities of ET-1.

MEASUREMENT RANGE

0.78 ~ 100 pg/mL

INTENDED USE

The IBL's ET-1 Assay Kit is a complete Kit for the quantitative determination of ET-1 in serum, EDTA-plasma, supernatant of cell culture media and the extracted solution from tissue.

KIT COMPONENT

1	Precoated plate	: Anti-ET ¹⁵⁻²¹ Rabbit IgG Affinity Purify	96Well x 1
2	Labeled antibody Conc.	: HRP conjugated Anti-ET-1 Rabbit IgG Fab' Affinity Purify (X30)	0.4mL x 1
3	Standard	: ET-1 (Peptide)	0.5mL x 2
4	EIA buffer	: 1% BSA, 0.05% Tween 20 in PBS	30mL x 1
5	Solution for Labeled antibody	: 1% BSA, 0.05% Tween 20 in PBS	12mL x 1
6	Chromogen	: TMB solution	15mL x 1
7	Stop solution	: 1N H ₂ SO ₄	12mL x 1
8	Wash buffer Conc.	: 0.05% Tween20 in phosphate buffer (X40)	50mL x 1

OPERATION MANUAL**1. Materials needed but not supplied**


- Plate reader (450nm)
- Graduated cylinder and beaker
- Incubator (37°C ± 1°C)
- Graph paper (log/log)
- Tube for dilution of Standard
- Disposable test tube for "2, Labeled antibody Conc." and "6, Chromogen"
- Micropipette and tip
- Distilled water
- Refrigerator (as 4°C)
- Paper towel
- Washing bottle for precoated plate

2. Preparation

- Preparation of wash buffer
"8, Wash buffer Conc." is a concentrated (X40) buffer. The temperature of "8, Wash buffer Conc." shall be adjusted to room temperature and then, mix it gently and completely before use. Dilute 50mL of "8, Wash buffer Conc." with 1,950mL of distilled water and mix it. This is the wash buffer for use. This prepared wash buffer shall be stored in refrigerator and used within 2 weeks after dilution.
- Preparation of Labeled antibody
"2, Labeled antibody Conc." is a concentrated (X30). Dilute "2, Labeled antibody Conc." with "5, Solution for Labeled antibody" in 30 times according to required quantity into a disposable test tube. Use this resulting solution as Labeled antibody.
Example)
In case you use one slit (8 well), the required quantity of Labeled antibody is 800 μL. (Dilute 30 μL of "2, Labeled antibody Conc." with 870 μL of "5, Solution for Labeled antibody" and mix it. And use the resulting solution by 100 μL in each well.)
This operation should be done just before the application of Labeled antibody.
The remaining "2, Labeled antibody Conc." should be stored at 4°C in firmly sealed vial.
- Preparation of Standard
Put just 0.5mL of distilled water into the vial of "3, Standard" and mix it gently and completely. This solution is 200 pg/mL ET-1 standard.
- Dilution of Standard
Prepare 9 tubes for dilution of "3, Standard". Put 230 μL each of "4, EIA buffer" into the tube.
Specify the following concentration of each tube.

Tube-1	100 pg/mL
Tube-2	50 pg/mL
Tube-3	25 pg/mL
Tube-4	12.5 pg/mL
Tube-5	6.25 pg/mL
Tube-6	3.13 pg/mL
Tube-7	1.56 pg/mL
Tube-8	0.78 pg/mL
Tube-9	0 pg/mL (Test Sample Blank)

Put 230 μL of Standard solution into tube-1 and mix it gently. Then, put 230 μL of tube-1 mixture into tube-2. Dilute two times standard solution in series to set up 8 points of diluted standard between 100 pg/mL and 0.78 pg/mL. "4, EIA buffer" is the test sample blank as 0 pg/mL.
See following picture.

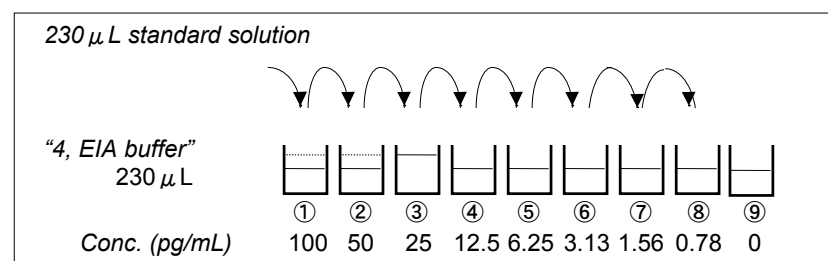

5) Dilution of test sample

Test sample may be diluted with "4, EIA buffer" if the need arises.

It is necessary to pre-extraction procedure by Sep-Pak C-18 column if you would like to apply serum, plasma or tissue samples. (see "Attention for sample handling" at the next page).

3. Measurement procedure

All reagents shall be brought to room temperature approximately 30 minutes before use. Then mix it gently and completely before use. Confirm no change in quality of the reagents. Standard curve shall be prepared simultaneously with the measurement of test samples.

Reagents	Test Sample	Standard	Test Sample Blank	Reagent Blank
	Test sample 100 μL	Diluted standard (Tube 1~8) 100 μL	EIA buffer (Tube-9) 100 μL	EIA buffer 100 μL
Incubation for overnight at 4°C with plate lid				
Washing 7 times				
Labeled Antibody	100 μL	100 μL	100 μL	-
Incubation for 30 minutes at 37°C with plate lid				
Washing 9 times				
Chromogen	100 μL	100 μL	100 μL	100 μL
Incubation for 30 minutes at room temperature (shielded)				
Stop solution	100 μL	100 μL	100 μL	100 μL
Read the plate at 450nm within 30 minutes after application of Stop solution.				

- Determine wells for reagent blank. Put 100 μL each of "4, EIA buffer" into the wells.
- Determine wells for test sample blank, test sample and diluted standard. Then, put 100 μL each of test sample blank (tube-9), test sample and dilutions of standard (tube-1~8) into the appropriate wells.
- Incubate the precoated plate for overnight at 4°C after covering it with plate lid.
- Wash each well of the precoated plate vigorously with wash buffer using washing bottle. Then, fill each well with wash buffer and place the precoated plate for 15~30 seconds. Remove wash buffer completely from the precoated plate by snapping.
This procedure must be repeated more than 7 times.
Then, remove the remaining liquid from all wells completely by snapping the precoated plate onto paper towel.
In case of using plate washer, after 4 times washing with plate washer, washing with above washing bottle must be repeated 3 times.
- Pipette 100 μL of labeled antibody solution into the wells of test samples, diluted standard and test sample blank.
- Incubate the precoated plate for 30 minutes at 37°C after covering it with plate lid.
- Wash the precoated plate 9 times in the same manner above 4).
- "6, Chromogen" should be taken the required quantity into a disposable test tube. Then, pipette 100 μL from the test tube into the wells. Please avoid to return the rest of test tube into "6, Chromogen" bottle due to avoid to cause of contamination.
- Incubate the precoated plate for 30 minutes at room temperature in the dark. The liquid will turn blue by the addition of "6, Chromogen".
- Pipette 100 μL of "7, Stop solution" into the wells. Mix the liquid by tapping the side of precoated plate. The liquid will turn yellow by the addition of "7, Stop solution".
- Remove any dirt or drop of water on the bottom of the precoated plate and confirm there is no bubble on the surface of the liquid. Then, run the plate reader and conduct measurement at 450nm.
The measurement shall be done within 30minutes after the addition of "7, Stop solution".

SPECIAL ATTENTION

- Test samples should be measured soon after the collection. In case of the storage of test samples, they should be stored under frozen conditions and do not repeat freeze/thaw cycles. Thaw the test samples at low temperature and mix them completely before measurement.
- Test samples should be diluted with "4, EIA buffer", if the need arises.
- The measurement of test samples and standard in duplicate is recommended.
- Use test samples in neutral pH range. The contaminations of organic solvent may affect the measurement.
- Use only wash buffer contained in this kit for washing the precoated plate. Insufficient washing may lead to the failure in measurement.
- Remove the wash buffer completely by tapping the precoated plate on paper towel.
Do not wipe wells with paper towel.
- "6, Chromogen" should be stored in the dark due to its sensitivity against light.

"6, Chromogen" should be avoided contact with metals.


8. Measurement should be done within 30 minutes after addition of "7, Stop solution".

CALCULATION OF TEST RESULT

Subtract the absorbance of test sample blank from all data, including standards and unknown samples before plotting. Plot the subtracted absorbance of the standards against the standard concentration on log-log graph paper. Draw the best smooth curve through these points to construct the standard curve. Read the concentration for unknown samples from the standard curve.

Example of standard curve

Conc. (pg/mL)	Absorbance (450nm)
100	2.868
50	1.750
25	0.969
12.5	0.566
6.25	0.339
3.13	0.225
1.56	0.169
0.78	0.137
0 (Test Sample Blank)	0.098

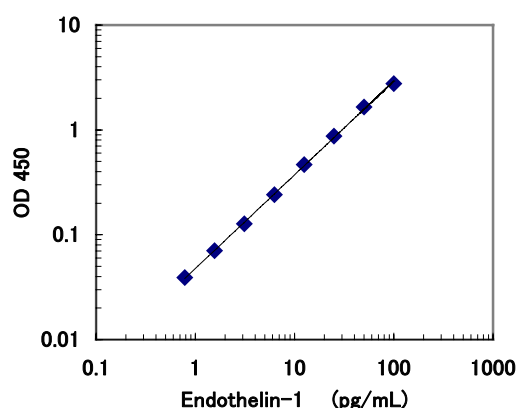

* The typical standard curve is shown above. This curve can not be used to derive test results. Please run a standard curve for each assay.

PERFORMANCE CHARACTERISTICS

(1) Titer Assay

Specimen	Titer (X)	Measurement Value (pg/mL)	Theoretical Value (pg/mL)	%
10% FCS added RPMI-1640	2	24.35	25.00	97.4
	4	12.36	12.50	98.9
	8	6.08	6.25	97.2
Human Serum	16	12.25	12.50	98.0
	32	6.47	6.30	103.5
	64	3.41	3.10	109.0
Human Plasma (EDTA)	4	9.33	13.00	74.7
	8	5.06	6.30	81.0
	16	2.92	3.13	93.5

(2) Added Recovery Assay

Specimen	Theoretical Value (pg/mL)	Measurement Value (pg/mL)	%
10% FCS added RPMI-1640 (x2)	25.03	25.49	101.8
	12.53	12.53	100.0
	6.28	5.86	93.3
Human Serum (x32)	25.11	20.46	81.5
	12.61	9.40	74.5
	6.36	4.52	71.0
Human Plasma (EDTA) (x8)	25.00	18.72	74.9
	12.50	9.34	74.7
	6.25	4.28	68.4

(3) Inter - Assay

Measurement Value (pg/mL)	SD value	CV value (%)	n
50.57	1.59	3.1	22
12.74	0.60	4.7	22
4.96	0.40	8.1	22

(4) Intra - Assay

Measurement Value (pg/mL)	SD value	CV value (%)	n
50.02	2.31	4.6	39
12.39	0.72	5.8	39
4.76	0.40	8.5	39

(5) Specificity

Compound	Cross Reactivity
Endothelin-1	100.0%
Endothelin-3	0.1%
Endothelin-1 (1-31)	≤0.1%
Endothelin-2 (1-31)	≤0.1%
Human Big Endothelin-1	≤0.1%
Rat Big Endothelin-1	≤0.1%

(6) Sensitivity

0.23 pg/mL

The sensitivity for this kit was determined using the guidelines under the National Committee for Clinical Laboratory Standards (NCCLS) Evaluation Protocols. (National Committee for Clinical Laboratory Standards Evaluation Protocols, SC1, (1989) Villanova, PA: NCCLS.

PRECAUTION FOR INTENDED USE AND/OR HANDLING

- All reagents should be stored at 2~8°C. All reagents shall be brought to room temperature approximately 30 minutes before use.
- "3, Standard" is lyophilized products. Be careful to open this vial.
- "7, Stop solution" is a strong acid substance. Therefore, be careful not to contact your skin and clothes with "7, Stop solution" and pay attention to the disposal of "7, Stop solution".
- "1, Precoated plate" and "3, Standard" contain sodium azide. Therefore, dispose these materials after diluting them with large quantity of water to avoid the production of explosive metallic azide.
- The precipitation may grow in "2, Labeled antibody Conc.", however, there is no problem in the performance.
- Wash hands after handling reagents.
- Do not mix the reagents with the reagents from different lot or different kit.
- Do not use the reagents expired.
- This kit is for research purpose only. Do not use for clinical diagnosis.

Attention for sample handling:

This kit will allow a direct assay samples containing a low concentration of protein (e.g. cell culture media, urine and so on). However, extraction and concentration of Endothelin from samples will be required for samples containing a high concentration of protein (e.g. plasma, tissue homogenates and so on). Extraction of test sample with Sep-Pak C-18 column is recommended as below:

- Pre-treatment of Sep-Pak C-18 column (*1)
 - Washing with 4mL of pure methanol.
 - Washing 2 times with 2mL of distilled water.
 - Washing 2 times with 2mL of 0.1% TFA solution
- Pre-treatment of samples
 - Plasma - Addition of 6mL of 10% CH₃COOH to 2mL of plasma with mixing
 - Tissue sample
 - Addition of 1M CH₃COOH - 20mM HCl solution to tissue sample and homogenize.
 - After boiling for ten minutes, centrifuge at 10,000rpm for 10min and collecting a supernatant.
- Extraction of sample
 - Addition of treated sample to Sep-Pak C-18 column.
 - Washing 3 times with 3mL of distilled water.
 - Elution with 2mL of an appropriate solution (*2) and collection to vial
- Measurement

Collected sample in vial should be lyophilized and stored under frozen condition until measurement. Stored sample should be reconstituted with 0.1mL of an appropriate solution (*3) and added 0.2mL of "4, EIA buffer" and mixed. Confirm that the pH of sample is in a neutral range before measurement. There is a difference in recovery rate between samples. Please test added recovery assay in advance.

(*1) Part No. 23501, manufactured by Waters Ltd. (U.S.A)

Amprep C2 column (Amersham Pharmacia Inc.) is also able to use instead of Sep-Pak C-18

(*2) 0.1% Trifluoroacetic Acid (*4) plus 60% Acetonitrile in dH₂O

(*3) 0.1% Trifluoroacetic Acid in DMSO

(*4) No. 206-10731, manufactured by Wako Pure Chemical Industries Ltd. (Japan) is used in our protocol.

STORAGE AND THE TERM OF VALIDITY

Storage Condition : 2 ~ 8°C

The term of validity : 12 months

(The expiry date is specified in outer box.)



REFERENCES

- Terui N, Suzuki H. CENTRAL NERVOUS SYSTEM AND BLOOD PRESSURE CONTROL 1992, *Proceedings of The 7th Workshop on "Brain and Blood Pressure Control"* p.141-148
- Tane N. et al. The effects of Endothelin-1 on Flap Necrosis. *Annals of Plastic Surgery*. 35(4) : 389-395, 1995.
- Wakisaka et al., Endothelin-1 kinetics in plasma urine, and blister fluid in burn patients. *Annals of Plastic Surgery*. 37, No.3, 305-309 1996

Version

041018 Established

Symbols / Symbole / Symbôles / Símbolos / Símbolos / Σύμβολα

	Cat.-No.: / Kat.-Nr.: / No.- Cat.: / Cat.-No.: / N.º Cat.: / N.-Cat.: / Αριθμός-Κατ.:
	Lot-No.: / Chargen-Bez.: / No. Lot: / Lot-No.: / Lote N.º: / Lotto n.: / Αριθμός -Παραγωγή:
	Use by: / Verwendbar bis: / Utiliser à: / Usado por: / Usar até: / Da utilizzare entro: / Χρησιμοποιείται από:
	No. of Tests: / Kitgröße: / Nb. de Tests: / No. de Determ.: / N.º de Testes: / Quantità dei tests: / Αριθμός εξετάσεων:
	Concentrate / Konzentrat / Concentré / Concentrar / Concentrado / Concentrato / Συμπύκνωμα
	Lyophilized / Lyophilisat / Lyophilisé / Liofilizado / Liofilizado / Liofilizzato / Λυοφιλιασμένο
	In Vitro Diagnostic Medical Device. / In-vitro-Diagnostikum. / Appareil Médical pour Diagnostics In Vitro. / Dispositivo Médico para Diagnóstico In Vitro. / Equipamento Médico de Diagnóstico In Vitro. / Dispositivo Medico Diagnostico In vitro. / Ιατρική συσκευή για In-Vitro Διάγνωση.
	Evaluation kit. / Nur für Leistungsbewertungszwecke. / Kit pour évaluation. / Juego de Reactivos para Evaluació. / Kit de avaliação. / Kit di valutazione. / Κιτ Αξιολόγησης.
	Read instructions before use. / Arbeitsanleitung lesen. / Lire la fiche technique avant emploi. / Lea las instrucciones antes de usar. / Ler as instruções antes de usar. / Leggere le istruzioni prima dell'uso. / Διαβάστε τις οδηγίες πριν την χρήση.
	Keep away from heat or direct sun light. / Vor Hitze und direkter Sonneneinstrahlung schützen. / Garder à l'abri de la chaleur et de toute exposition lumineuse. / Manténgase alejado del calor o la luz solar directa. / Manter longe do calor ou luz solar directa. / Non esporre ai raggi solari. / Να φυλάσσεται μακριά από θερμότητα και άμεση επαφή με το φως του ηλίου.
	Store at: / Lagern bei: / Stocker à: / Almacene a: / Armazenar a: / Conservare a: / Αποθήκευση στους:
	Manufacturer: / Hersteller: / Fabricant: / Productor: / Fabricante: / Fabricante: / Παραγωγός:
	Caution! / Vorsicht! / Attention! / ¡Precaución! / Cuidado! / Attenzione! / Προσοχή!
<p>Symbols of the kit components see MATERIALS SUPPLIED. Die Symbole der Komponenten sind im Kapitel KOMPONENTEN DES KITS beschrieben. Voir MATERIEL FOURNI pour les symbôles des composants du kit. Símbolos de los componentes del juego de reactivos, vea MATERIALES SUMINISTRADOS. Para símbolos dos componentes do kit ver MATERIAIS FORNECIDOS. Per i simboli dei componenti del kit si veda COMPONENTI DEL KIT. Για τα σύμβολα των συστατικών του κιτ συμβουλευτείτε το ΠΑΡΕΧΟΜΕΝΑ ΥΛΙΚΑ.</p>	

IBL AFFILIATES WORLDWIDE

IBL International GmbH Flughafenstr. 52A, 22335 Hamburg, Germany	Tel.: + 49 (0) 40 532891 -0 Fax: -11 E-MAIL: IBL@IBL-International.com WEB: http://www.IBL-International.com
IBL International B.V. Zuthpenseweg 55, 7418 AH Deventer, The Netherlands	Tel.: + 49 (0) 40 532891 -0 Fax: -11 E-MAIL: IBL@IBL-International.com WEB: http://www.IBL-International.com
IBL International Corp. 194 Wildcat Road, Toronto, Ontario M3J 2N5, Canada	Tel.: +1 (416) 645 -1703 Fax: -1704 E-MAIL: Sales@IBL-International.com WEB: http://www.IBL-International.com

LIABILITY: Complaints will be accepted in each mode –written or vocal. Preferred is that the complaint is accompanied with the test performance and results. Any modification of the test procedure or exchange or mixing of components of different lots could negatively affect the results. These cases invalidate any claim for replacement. Regardless, in the event of any claim, the manufacturer's liability is not to exceed the value of the test kit. Any damage caused to the kit during transportation is not subject to the liability of the manufacturer.