

Melatonin ELISA

Enzyme immunoassay for the quantitative determination of melatonin in human serum and plasma.

REF **RE54021**

 **96**

   **2-8°C**

EU: **IVD** 



I B L I N T E R N A T I O N A L G M B H

Flughafenstrasse 52a
D-22335 Hamburg, Germany

Phone: +49 (0)40-53 28 91-0
Fax: +49 (0)40-53 28 91-11

IBL@IBL-International.com
www.IBL-International.com

1. INTENDED USE

Enzyme immunoassay for the quantitative determination of melatonin in human serum and plasma.

2. SUMMARY AND EXPLANATION

The pineal gland (corpus pineale) has been called a neuroendocrine transducer because of its important role in photoperiodism. The major hormone of the pineal gland is N-acetyl-5-methoxy-tryptamine or melatonin which is synthesized from the amino acid tryptophane. Melatonin has its highest levels in plasma during nighttime. Its characteristic nocturnal surge appears to encode temporal information such as length of night. Regulation of the melatonin secretion is under neural control. Sympathetic innervation seems to play a major role via its release of noradrenaline. Altered patterns and/or levels of melatonin secretion have been reported to coincide with sleep disorders, jet lag, depression, stress, schizophrenia, hypothalamic amenorrhea, pregnancy, anorexia nervosa, some forms of cancer, immunological disorders as well as control of sexual maturation during puberty.

Most of the circulating melatonin is metabolized in the liver to 6-hydroxymelatonin and subsequently to 6-sulfatoxymelatonin which is excreted into the urine.

The concentration of 6-hydroxymelatonin sulfate in urine correlates well with the total level of melatonin in the blood during the collection period.

3. TEST PRINCIPLE

The assay procedure follows the basic principle of competitive ELISA whereby there is competition between a biotinylated and a non-biotinylated antigen for a fixed number of antibody binding sites. The amount of biotinylated antigen bound to the antibody is inversely proportional to the analyte concentration of the sample. When the system is in equilibrium, the free biotinylated antigen is removed by a washing step and the antibody bound biotinylated antigen is determined by use of streptavidine alkaline phosphatase as marker and p-nitrophenyl phosphate as substrate. Quantification of unknowns is achieved by comparing the enzymatic activity of unknowns with a response curve prepared by using known standards.

4. WARNINGS AND PRECAUTIONS

1. For *in-vitro diagnostic* use only. For professional use only.
2. Before starting the assay, read the instructions completely and carefully. Use the valid version of the package insert provided with the kit. Be sure that everything is understood.
3. In case of severe damage of the kit package please contact IBL or your supplier in written form, latest one week after receiving the kit. Do not use damaged components in test runs, but keep safe for complaint related issues.
4. Obey lot number and expiry date. Do not mix reagents of different lots. Do not use expired reagents.
5. Follow good laboratory practice and safety guidelines. Wear lab coats, disposable latex gloves and protective glasses where necessary.
6. Reagents of this kit containing hazardous material may cause eye and skin irritations. See MATERIALS SUPPLIED and labels for details. Material Safety Data Sheets for this product are available on the IBL-Homepage or upon request directly from IBL.
7. Chemicals and prepared or used reagents have to be treated as hazardous waste according to national biohazard and safety guidelines or regulations.
8. The cleaning staff should be guided by the professionals regarding potential hazards and handling.
9. Avoid contact with Stop solution. It may cause skin irritations and burns.
10. All reagents of this kit containing human serum or plasma have been tested and were found negative for anti-HIV I/II, HBsAg and anti-HCV. However, a presence of these or other infectious agents cannot be excluded absolutely and therefore reagents should be treated as potential biohazards in use and for disposal.

5. STORAGE AND STABILITY

The kit is shipped at ambient temperature and should be stored at 2-8 °C. Keep away from heat or direct sun light. The storage and stability of specimen and prepared reagents is stated in the corresponding chapters.

The microtiter strips are stable up to the expiry date of the kit in the broken, but tightly closed bag when stored at 2–8 °C.

After elution with methanol the Extraction Columns may be used for extraction of the next samples or stored at 2-8°C protected from dust. Extraction Columns may be re-used up to 4 times.

6. SPECIMEN COLLECTION AND STORAGE

Serum, Plasma (EDTA, Heparin)

The usual precautions for venipuncture should be observed. It is important to preserve the chemical integrity of a blood specimen from the moment it is collected until it is assayed. Do not use grossly hemolytic, icteric or grossly lipemic specimens. Samples appearing turbid should be centrifuged before testing to remove any particulate material.

Storage:	2-8°C	≤ -20°C (Aliquots)	≤ -70°C (Aliquots)	Keep away from heat or direct sun light. Avoid repeated freeze-thaw cycles.
Stability:	24 h	3 months	12 months	

7. MATERIALS SUPPLIED



The reagents provided with this kit are sufficient for single determinations in the sample preparation (extraction) and duplicates in the assay. Additional reagents are available upon request.

Quantity	Symbol	Component
1 x 12x8	MTP	Microtiter Plate Break apart strips. Coated with anti-rabbit IgG (goat, polyclonal).
3 x 2 mL	BIOTIN LYO	Melatonin Biotin , lyophilized Contains: stabilizers.
3 x 2 mL	ANTISERUM LYO	Melatonin Antiserum , lyophilized Contains: Antiserum (rabbit, polyclonal), stabilizers.
1 x 250 µL	ENZCONJ CONC	Enzyme Conjugate , Concentrate (80x). Contains: streptavidin alkaline phosphatase, Tris buffer, stabilizers.
1 x 6 x 2 mL	CAL A-F LYO	Standard A-F , lyophilized Contains: stabilizers. For exact concentrations see vial labels or QC Certificate.
1 x 2 x 2 mL	CONTROL 1+2 LYO	Control 1+2 , lyophilized Contains: stabilizers. Concentrations / acceptable ranges see QC Certificate.
1 x 100 mL	WASHBUF CONC	Wash Buffer , Concentrate (10x) Contains: phosphate buffer.
2 x 13 mL	PNPP SUBS	PNPP Substrate Solution Ready to use. Contains: p-nitrophenyl phosphate (PNPP).
1 x 15 mL	PNPP STOP	PNPP Stop Solution Ready to use. Contains: 1 M NaOH, 0.25 M EDTA.
2 x 10	EXTRCOL	Extraction Columns Ready to use. C18 RP. 1 cm ³ /100 mg. Additional extraction columns can be ordered separately from IBL under REF KEME761.
3 x	FOIL	Adhesive Foil


8. MATERIALS REQUIRED BUT NOT SUPPLIED

1. Micropipettes (Multipette Eppendorf or similar devices, < 3 % CV). Volume: 50; 500 µL
2. Disposable glass test tubes or round-bottom polystyrene test tubes (12 x 75 mm)
3. Orbital shaker (400-600 rpm)
4. Vortex mixer
5. 8-Channel Micropipettor with reagent reservoirs
6. Wash bottle, automated or semi-automated microtiter plate washing system
7. Centrifuge; 100-200 x g
alternatively: Vacuum manifold (e.g. Mallinckrodt-Baker or Waters)
8. Methanol (HPLC grade)
9. Evaporator centrifuge (Speed-Vac)
alternatively: Sample concentrator by use of nitrogen (e.g. Techne)
10. Microtiter plate reader capable of reading absorbance at 405 nm (reference wavelength 600-650 nm)
11. Bidistilled or deionised water
12. Paper towels, pipette tips and timer

9. PROCEDURE NOTES

- Any improper handling of samples or modification of the test procedure may influence the results. The indicated pipetting volumes, incubation times, temperatures and pretreatment steps have to be performed strictly according to the instructions. Use calibrated pipettes and devices only.
- Once the test has been started, all steps should be completed without interruption. Make sure that required reagents, materials and devices are prepared ready at the appropriate time. Allow all reagents and specimens to reach room temperature (18-25 °C) and gently swirl each vial of liquid reagent and sample before use. Mix reagents without foaming.
- Avoid contamination of reagents, pipettes and wells/tubes. Use new disposable plastic pipette tips for each component and specimen. Do not interchange caps. Always cap not used vials. Do not reuse wells/tubes or reagents.
- It is advised to determine samples in duplicate to be able to identify potential pipetting errors.
- Use a pipetting scheme to verify an appropriate plate layout.
- Incubation time affects results. All wells should be handled in the same order and time sequences. It is recommended to use an 8-channel Micropipettor for pipetting of solutions in all wells.
- Microplate washing is important. Improperly washed wells will give erroneous results. It is recommended to use a multichannel pipette or an automatic microplate washing system. Do not allow the wells to dry between incubations. Do not scratch coated wells during rinsing and aspiration. Rinse and fill all reagents with care. While rinsing, check that all wells are filled precisely with Wash Buffer, and that there are no residues in the wells.
- Humidity affects the coated wells/tubes. Do not open the pouch until it reaches room temperature. Unused wells/tubes should be returned immediately to the resealed pouch including the desiccant.
- The relative centrifugal force (g) is not equivalent to rounds per minute (rpm) but it has to be calculated depending on the radius of the centrifuge.

10. PRE-TEST SETUP INSTRUCTIONS

	The contents of the kit for 96 determinations can be divided into 3 separate runs. The volumes stated below are for one run with 4 strips (32 determinations).
---	--

10.1. Preparation of lyophilized or concentrated components

Dilute / dissolve	Component		Diluent	Relation	Remarks	Storage	Stability
15 mL	WASHBUF	ad 150 mL	bidist. water	1:10	Warm up at 37°C to dissolve crystals, if necessary. Mix vigorously.	2-8 °C	8 weeks
	CAL A-F CONTROL 1+2	with 2.0 mL	bidist. water		Let stand for 15 min. Mix without foaming.	≤ -20 °C (Aliquots)	until Exp. date
	BIOTIN	with 2.0 mL	WASHBUF (diluted)		Let stand for 15 min. Mix without foaming.	Prepare freshly and use only once.	
	ANTISERUM	with 2.0 mL	bidist. water		Let stand for 15 min. Mix without foaming.		
70 µL	ENZCONJ	with 5.6 mL	WASHBUF (diluted)	1:81			
10 mL	Methanol (undiluted)	ad 100 mL	bidist. water	10 % (v/v)			

If a larger volume is needed, vials can be pooled. Avoid repeated freeze-thaw cycles.


10.2. Dilution of Samples

Samples suspected to contain concentrations higher than the highest standard have to be diluted with diluted Wash Buffer prior to extraction step.

10.3. Extraction of Samples, Standards and Controls (Extraction Column)

The yield of extraction with this procedure is approx. 90-100 %.

Filter or centrifuge the samples prior to extraction in order to avoid clogging of the columns.

	<p>Each sample, Standard and Control has to be extracted. Extraction may be performed in advance. The dried extracts (after evaporation of methanol) may be stored at 2-8 °C or ≤ -20 °C for up to 24 h.</p> <p>After elution with methanol the Extraction Columns may be used for extraction of the next samples or stored at 2-8 °C protected from dust. Extraction Columns may be re-used up to 4 times. In case of re-use, start again with A.1 (Column Conditioning).</p>
---	--

A. Standard version: Procedure for Centrifuge and Evaporator Centrifuge

1. Column Conditioning:

1.	Place the Extraction Columns into polystyrene or glass tubes (12 x 75 mm).
2.	Add 1 x 1 mL of methanol (undiluted) to the columns. Let the solvent pass through the column by centrifugation for 1 min at 120 x g. Discard eluate.
3.	Add 1 x 1 mL of bidist. water to the columns. Let the solvent pass through the column by centrifugation for 1 min at 120 x g. Discard eluate.
4.	Proceed with sample application without delay in order to avoid the columns getting dry.

2. Sample Application:

5.	Place the Extraction Columns into correspondingly marked polystyrene or glass tubes (12 x 75 mm).
6.	Add 0.5 mL of Standards, Controls and samples to the columns.
7.	Add 0.5 mL of bidist. water to the columns. Let pass through the column by centrifugation for 5 min at 120 x g. Discard eluate.

3. Washing:

8.	Add 2 x 1 mL of 10 % methanol in bidist. water (v/v) to the columns. Let the solvent pass through the column by centrifugation for 5 min at 120 x g. Discard eluate.
----	---

4. Elution of Extract:

9.	Place the Extraction Columns into new, correspondingly marked polystyrene or glass tubes (12 x 75 mm).
10.	Add 1 mL of methanol (undiluted) to the columns. Let the solvent pass through the column by centrifugation for 5 min at 120 x g.
11.	Remove columns from the tubes. Avoid drops to be left at the columns. Use columns for extraction of the next samples or store at 2-8 °C protected from dust. Extraction Columns may be re-used up to 4 times.

5. Evaporation and Reconstitution of Extract:

12.	Evaporate the methanol to dryness by use of evaporator centrifuge.
13.	Reconstitute samples with 0.15 mL of bidist. water .
14.	Vortex at least 1 min and assay immediately.

B. Alternative version: Procedure for Vacuum Manifold instead of a Centrifuge

For the extraction scheme follow points A 1-5 accordingly. The volumes remain unchanged.

Let the **solvent** pass through the column using vacuum and a flow rate of ≤ 5 mL/min.

For the **samples and extracts** use a flow rate of ≤ 2 mL/min.

The evaporation of the solvent may be performed by using an evaporator centrifuge or by nitrogen.

11. TEST PROCEDURE

1.	Pipette 50 µL of each <u>extracted</u> Standard , <u>extracted</u> Control and <u>extracted</u> sample into the respective wells of the Microtiter Plate.
2.	Pipette 50 µL of Melatonin Biotin into each well.
3.	Pipette 50 µL of Melatonin Antiserum into each well.
4.	Cover plate with adhesive foil. Shake plate carefully. Incubate 14-20 h at 2-8 °C .
5.	Remove adhesive foil. Discard incubation solution. Wash plate 3 x with 250 µL of diluted Wash Buffer . Remove excess solution by tapping the inverted plate on a paper towel.
6.	Pipette 150 µL of freshly prepared Enzyme Conjugate into each well.
7.	Cover plate with new adhesive foil. Incubate 120 min at RT (18-25 °C) on an orbital shaker (500 rpm).
8.	Remove adhesive foil. Discard incubation solution. Wash plate 3 x with 250 µL of diluted Wash Buffer . Remove excess solution by tapping the inverted plate on a paper towel.
9.	For adding of Substrate and Stop Solution use, if available, an 8-channel Micropipettor. Pipetting should be carried out in the same time intervals for Substrate and Stop Solution. Use positive displacement and avoid formation of air bubbles.
10.	Pipette 200 µL of PNPP Substrate Solution into each well.
11.	Incubate 40 min at RT (18-25 °C) on an orbital shaker (500 rpm).
12.	Stop the substrate reaction by adding 50 µL of PNPP Stop Solution into each well. Briefly mix contents by gently shaking the plate.
13.	Measure optical density with a photometer at 405 nm (Reference-wavelength: 600-650 nm) within 60 min after pipetting of the Stop Solution.

12. QUALITY CONTROL

The test results are only valid if the test has been performed following the instructions. Moreover the user must strictly adhere to the rules of GLP (Good Laboratory Practice) or comparable standards/laws. User and/or laboratory must have a validated system to get diagnosis according to GLP. All kit controls must be found within the acceptable ranges as stated on the labels and the QC certificate. If the criteria are not met, the run is not valid and should be repeated. Each laboratory should use known samples as further controls. It is recommended to participate at appropriate quality assessment trials.

In case of any deviation the following technical issues should be proven: Expiration dates of (prepared) reagents, storage conditions, pipettes, devices, incubation conditions and washing methods.

13. CALCULATION OF RESULTS

The obtained OD of the standards (y-axis, linear) are plotted against their concentration (x-axis, logarithmic) either on semi-logarithmic graph paper or using an automated method. A good fit is provided with cubic spline, 4 Parameter Logistics or Logit-Log.

For the calculation of the standard curve, apply each signal of the standards (one obvious outlier of duplicates might be omitted and the more plausible single value might be used).

The concentration of the samples can be read directly from the standard curve.

In case of diluted samples the values have to be multiplied with the corresponding dilution factor.

Samples showing concentrations above the highest standard have to be diluted as described in PRE-TEST SETUP INSTRUCTIONS and reassayed.

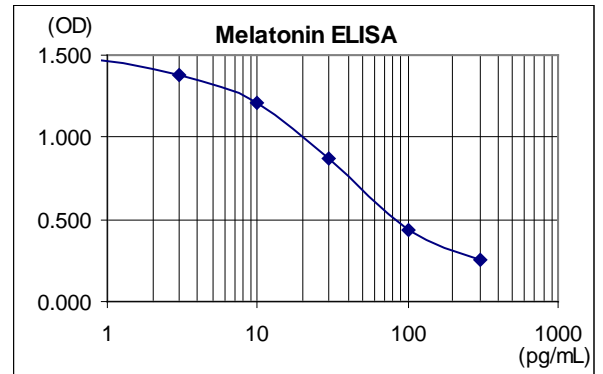
Conversion:

Melatonin (pg/mL) x 4.30 = pmol/L

Typical Calibration Curve

(Example. Do not use for calculation!)

Standard	Melatonin (pg/mL)	OD _{Mean}	OD/OD _{max} (%)
A	0.0	1.517	100.0
B	3.0	1.383	91.1
C	10	1.214	80.1
D	30	0.867	57.1
E	100	0.434	28.6
F	300	0.260	17.1

**14. EXPECTED VALUES**

The results themselves should not be the only reason for any therapeutic consequences. They have to be correlated to other clinical observations and diagnostic tests.

A study with apparently healthy subjects has shown that the melatonin levels in humans have a marked circadian rhythmicity characterised by very low levels during day-time and high levels during night-time, and show a considerable inter-individual variation. Furthermore, the melatonin concentration is age dependent. The highest concentrations were found in samples of infants (up to 3 years).

In a group of six healthy volunteers the circadian rhythm of melatonin was studied. The mean value reaches a minimum of about 4.6 pg/mL during daytime at 4 p.m. and a maximum of about 77.5 pg/mL during night-time at 4 a.m. The nocturnal melatonin peak among healthy individuals varies significantly.

Melatonin in Serum

Apparently healthy subjects show the following values:

Time	n	Mean Melatonin in Serum	90% percentile
03:00 A.M.	129	78.2 pg/mL	18.5-180 pg/mL
08:00 A.M.	128	28.5 pg/mL	3.8-80.4 pg/mL

Reference: Terzieva et al. Clin Lab (2009)

It is recommended that each laboratory establishes its own range of normal values.

15. LIMITATIONS OF THE PROCEDURE

Specimen collection has a significant effect on the test results. See SPECIMEN COLLECTION AND STORAGE for details.

For cross-reactivities, see PERFORMANCE.

The following blood components do not have a significant effect (+/-20% of expected) on the test results up to the below stated concentrations:

Hemoglobin	8.0 mg/mL
Bilirubin	0.36 mg/mL














16. PERFORMANCE

Analytical Specificity (Cross Reactivity)	Substance	Cross Reactivity (%)		Cross-reactivity of other substances tested < 0.01 %
	5-Methoxy-Tryptophole	1.2		
	N-Acetyl-Serotonin	1.2		
	5-Methoxy-Tryptamine	2.5		
Analytical Sensitivity (Limit of Detection)	1.6 pg/mL	Mean signal (Zero-Standard) - 2SD		
Precision	Range (pg/mL)	CV (%)		
Intra-Assay	8.8 – 151.7	3.0 – 11.4		
Inter-Assay	5.6 – 134.3	6.4 – 19.3		
Linearity	Range (pg/mL)	Serial dilution up to		Range (%)
	80.7 – 191.4	1:16		73 - 135
Recovery	Mean (%)	Range (%)		% Recovery after spiking
	102.4	83 - 125		
Method Comparison versus IBL RIA	IBL ELISA = 1.01 x IBL RIA + 4.6			r = 0.98; n = 50
Method Comparison versus other RIA	IBL ELISA = 0.86 x other RIA + 5.33			r = 0.96; n = 46

17. PRODUCT LITERATURE REFERENCES

1. Terzieva, DD, Mateva ND, Vladimirova-Kitova LG: Melatonin reference limits at 3:00 AM and 8:00 AM in healthy adults. Clin. Lab. 55:359-361 (2009)
2. Iriti, M., Rossoni, M, Faoro F. Melatonin content in grape myth or panacea? J Sci Food Agric 86:1432-1438 (2006)
3. Lahiri, D. K., Ge, Y.-W., Sharman, E. H., Bondy, St. C., Age-related changes in serum melatonin in mice: higher levels of combined melatonin and 6-hydroxymelatonin sulfate in the cerebral cortex than serum, heart, liver and kidney tissues. J. Pineal Res. May 2004, Vol. 36, issue 4, 217-223
4. Sharman E et al. Age-related changes in murine CNS mRNA gene expression are modulated by dietary melatonin. J. Pineal Res. Vol 36, Issue 3: 165ff. (2004)
5. Wagner H.-J. Mattheus U. Pineal organs in deep demersal fish. Cell Tissue Res 307:115-127 (2002)
6. Kunz D et al. Melatonin as a therapy in REM sleep behavior disorder patients: an open-labeled pilot study on the possible influence of melatonin on REM-sleep regulation. Movement Disorders, 14: 507-511 (1999)
7. Pflugger DH, Minder CE. Effects of exposure to 16.7 Hz magnetic fields on urinary 6-hydroxymelatonin sulfate excretion of Swiss railway workers. J. Pineal Res., 21: 91-100 (1996)
8. Follenius M, Weibel L, Brandenberger G. Distinct modes of melatonin secretion in normal men. J. Pineal Res., 18: 135-140 (1995)
9. Dubbels R et al. Melatonin in edible plants identified by radioimmunoassay and by high performance liquid chromatography-mass spectrometry. J. Pineal Res., 18. 28-31 (1995)
10. Czeisler CA et al. Suppression of melatonin secretion in some blind patients by exposure to bright light. N. Engl. J. Med., 332: 6-11 (1995)

Symbols / Symbole / Symbôles / Símbolos / Símbolos / Σύμβολα

	Cat.-No.: / Kat.-Nr.: / No.- Cat.: / Cat.-No.: / N.º Cat.: / N.-Cat.: / Αριθμός-Κατ.:
	Lot-No.: / Chargen-Bez.: / No. Lot: / Lot-No.: / Lote N.º: / Lotto n.: / Αριθμός -Παραγωγή:
	Use by: / Verwendbar bis: / Utiliser à: / Usado por: / Usar até: / Da utilizzare entro: / Χρησιμοποιείται από:
	No. of Tests: / Kitgröße: / Nb. de Tests: / No. de Determ.: / N.º de Testes: / Quantità dei tests: / Αριθμός εξετάσεων:
	Concentrate / Konzentrat / Concentré / Concentrar / Concentrado / Concentrato / Συμπύκνωμα
	Lyophilized / Lyophilisat / Lyophilisé / Liofilizado / Liofilizado / Liofilizzato / Λυοφιλιασμένο
	In Vitro Diagnostic Medical Device. / In-vitro-Diagnostikum. / Appareil Médical pour Diagnostics In Vitro. / Dispositivo Médico para Diagnóstico In Vitro. / Equipamento Médico de Diagnóstico In Vitro. / Dispositivo Medico Diagnostico In vitro. / Ιατρική συσκευή για In-Vitro Διάγνωση.
	Evaluation kit. / Nur für Leistungsbewertungszwecke. / Kit pour évaluation. / Juego de Reactivos para Evaluació. / Kit de avaliação. / Kit di evaluazione. / Κιτ Αξιολόγησης.
	Read instructions before use. / Arbeitsanleitung lesen. / Lire la fiche technique avant emploi. / Lea las instrucciones antes de usar. / Ler as instruções antes de usar. / Leggere le istruzioni prima dell'uso. / Διαβάστε τις οδηγίες πριν την χρήση.
	Keep away from heat or direct sun light. / Vor Hitze und direkter Sonneneinstrahlung schützen. / Garder à l'abri de la chaleur et de toute exposition lumineuse. / Manténgase alejado del calor o la luz solar directa. / Manter longe do calor ou luz solar directa. / Non esporre ai raggi solari. / Να φυλάσσεται μακριά από θερμότητα και άμεση επαφή με το φως του ηλίου.
	Store at: / Lagern bei: / Stocker à: / Almacene a: / Armazemar a: / Conservare a: / Αποθήκευση στους:
	Manufacturer: / Hersteller: / Fabricant: / Productor: / Fabricante: / Fabbicante: / Παραγωγός:
	Caution! / Vorsicht! / Attention! / ¡Precaución! / Cuidado! / Attenzione! / Προσοχή!
<p>Symbols of the kit components see MATERIALS SUPPLIED. Die Symbole der Komponenten sind im Kapitel KOMPONENTEN DES KITS beschrieben. Voir MATERIEL FOURNI pour les symbôles des composants du kit. Símbolos de los componentes del juego de reactivos, vea MATERIALES SUMINISTRADOS. Para símbolos dos componentes do kit ver MATERIAIS FORNECIDOS. Per i simboli dei componenti del kit si veda COMPONENTI DEL KIT. Για τα σύμβολα των συστατικών του κιτ συμβουλευτείτε το ΠΑΡΕΧΟΜΕΝΑ ΥΛΙΚΑ.</p>	

COMPLAINTS: Complaints may be submitted initially written or vocal. Subsequently they need to be filed including the test performance and results in writing in case of analytical reasons.

WARRANTY: The product is warranted to be free from material defects within the specific shelf life and to comply with product specifications delivered with the product. The product must be used according to the Intended use, all instructions given in the instructions for use and within the product specific shelf life. Any modification of the test procedure or exchange or mixing of components of different lots could negatively affect the results. These cases invalidate any claim for replacement.

LIMITATION OF LIABILITY: IN ALL CIRCUMSTANCES THE EXTENT OF MANUFACTURER'S LIABILITY IS LIMITED TO THE PURCHASE PRICE OF THE KIT(S) IN QUESTION. IN NO EVENT SHALL MANUFACTURER BE LIABLE FOR ANY INCIDENTAL OR CONSEQUENTIAL DAMAGES, INCLUDING DAMAGES FOR LOST PROFITS, LOST SALES, INJURY TO PERSON OR PROPERTY OR ANY OTHER INCIDENTAL OR CONSEQUENTIAL LOSS.

	IBL International GmbH	Tel.: + 49 (0) 40 532891 -0	Fax: -11
	Flughafenstr. 52A, 22335 Hamburg, Germany	E-MAIL: IBL@IBL-International.com	
		WEB: http://www.IBL-International.com	