




Performance Data for Some POC HbA1c Systems: *Devices Are Similar to Central Laboratory Standards*

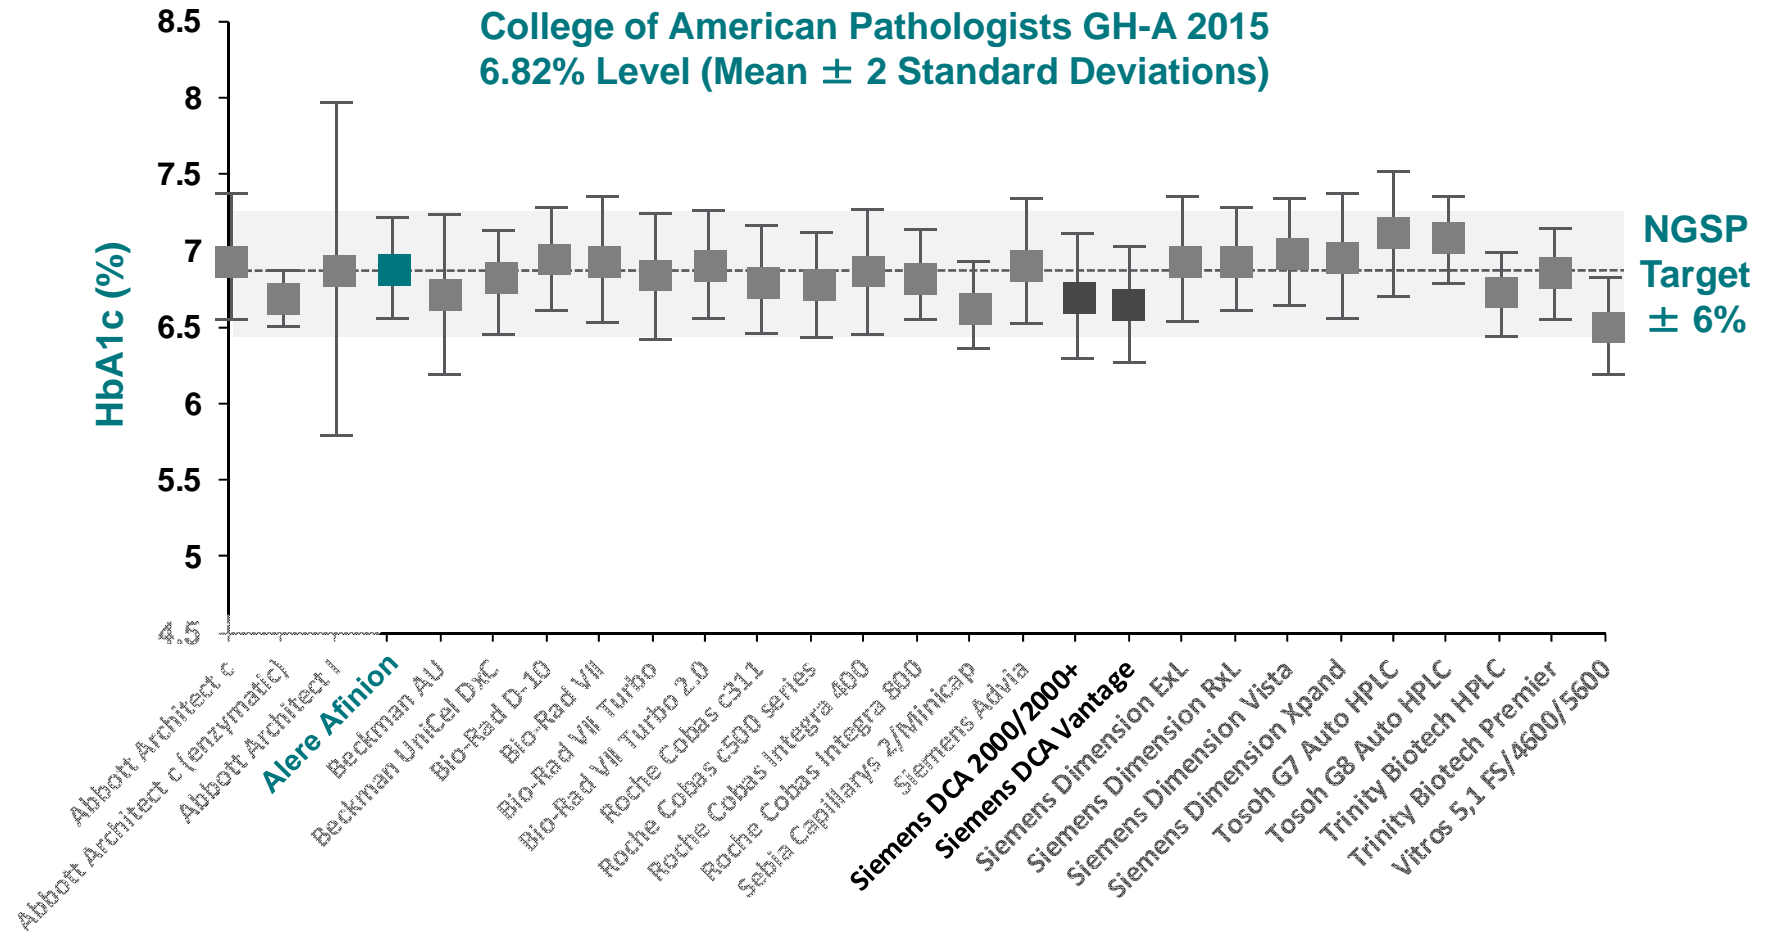

Alere Afinion, Siemens DCA 2000
and **Siemens DCA Vantage** are POC

Permission granted from: NGSP = National Glycohemoglobin Standardization Program
<http://www.ngsp.org/CAP/CAP15a.pdf>. Accessed 09/23/15.